

Aerosol Mass Spectrometer Measurements-MS20020721.TO

Figure 1. Sulfate mass concentration ($\mu\text{g}/\text{m}^3$, STP)

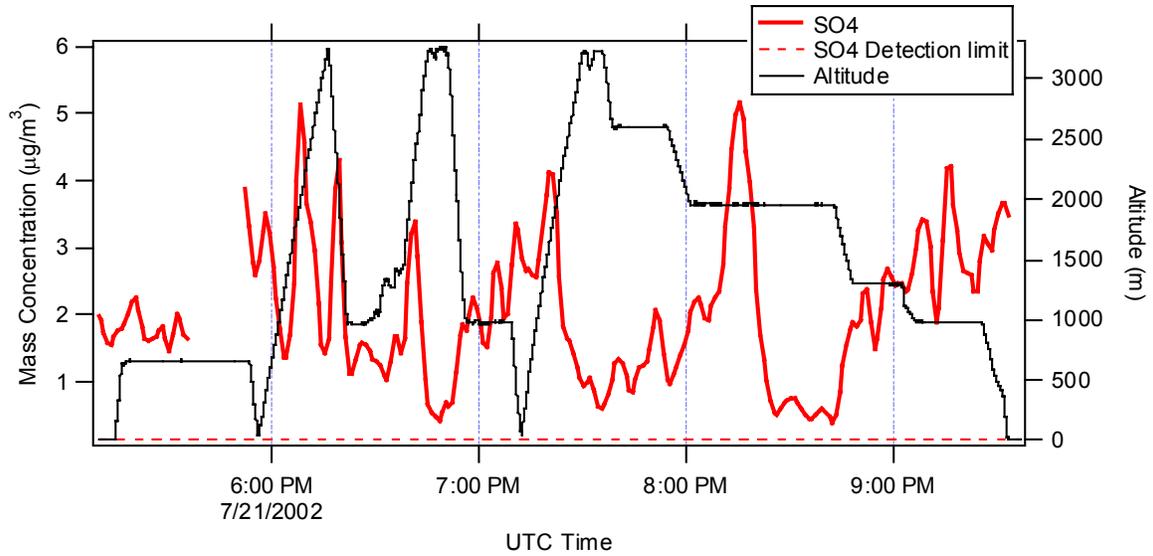


Figure 2. Nitrate mass concentration ($\mu\text{g}/\text{m}^3$, STP)

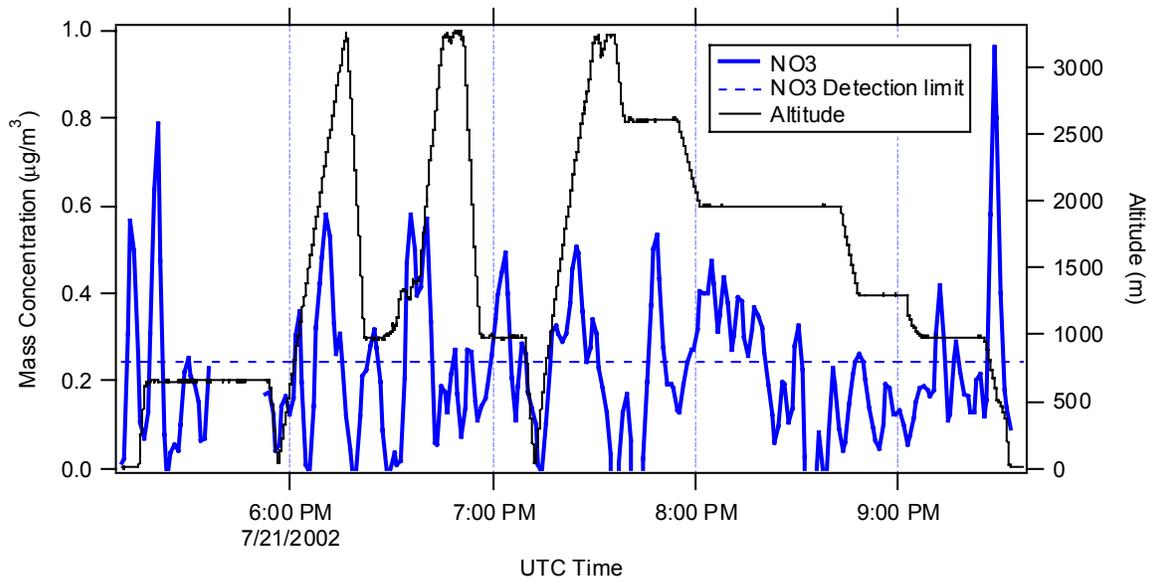


Figure 3. Organics mass concentration ($\mu\text{g}/\text{m}^3$, STP)

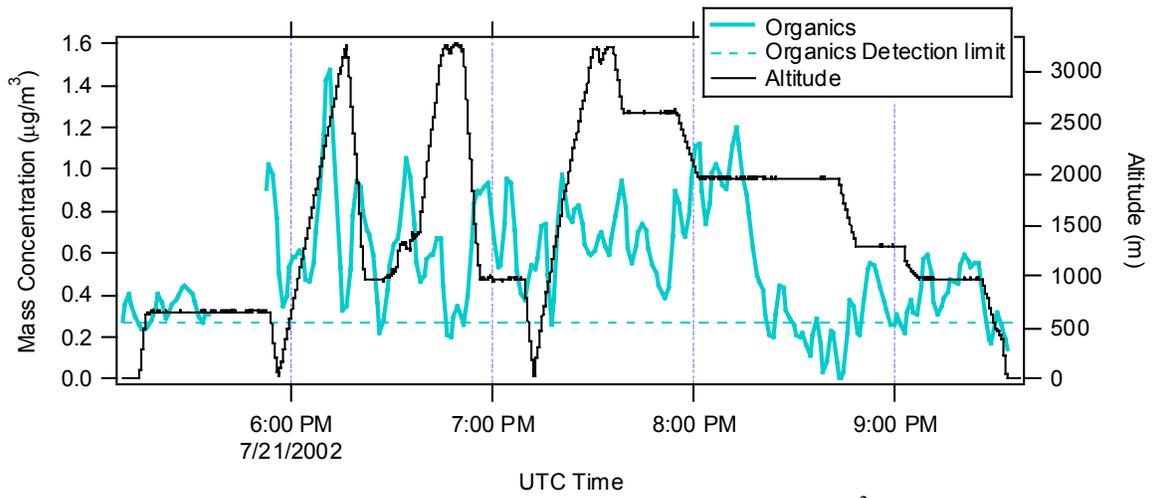


Figure 4. Preliminary Sulfate mass distribution ($dM/d\text{Log}D_a$, $\mu\text{g}/\text{m}^3$)

